

# Intelligent Series Gas Sensors (iseries)

Combustible Gases and Vapours (LEL) Sensor  
 Part Numbers: PM 979-600D-CIT (for iLEL75);  
 PM 989-600D-CIT (for iLEL75C);  
 PM 999-600D-CIT (for iLEL75M)

## Document Purpose

The purpose of this document is to present the performance specification of the intelligent iLEL75 combustible gases and vapours gas sensor. This document should be used in conjunction with the Product Safety Datasheet (PSDS 22). For guidance on the safe use of the sensor, please refer to the User's manual and application note (for mounting and sealing around sensor).



## KEY FEATURES & BENEFITS



### Digital interface

The sensor has a UART protocol to communicate with the instrument with chip select option as described in technical note.



### Interchangeable

All intelligent sensors have the same dimensions and communication protocol.

Supply voltage of all sensors is in the range from 3.1 V to 3.3 V.



### Digital traceability

Sensors contain the following data: serial number, manufacturing date, and gas type for quick and easy identification of the sensor.



### OEM lock

Sensors have two levels of lock codes. The first one is an OEM specific code programmed in during manufacture and cannot be modified. This lock code is provided by the OEM. Instrument can check if the sensor has the unique code - if not the instrument can refuse the sensor. The second level of lock code is left blank and can be updated by OEM/Partners during sensor integration into the instrument as needed.



### Designed to meet global performance standards

**Compliance with** EN IEC 60079-0, EN 60079-1, EN 60079-11, EN 50303 & EN 50270

**ATEX certificate number:** DEMKO 16 ATEX 1557U Rev. 2

**Designed to meet performance standards.** Consult page 4 and 5 for a full list of the applicable standards and ATEX marking.



### Pre-calibrated

Sensors will be calibrated during manufacturing and calibration data is written in the sensor. Sensor will output gas concentration when interrogated by instrument.

**RoHS**

RoHS compliant



5-year life



Compact form-fit

### LEL SENSOR VARIANTS

| SENSOR                    | iLEL75                        | iLEL75C                                      | iLEL75M  |
|---------------------------|-------------------------------|--|--|
| <b>Target Gas</b>         | Combustible gases and vapours | Combustible gases and vapours up to C6       | Methane and hydrogen                               |
| <b>Inboard Filter</b>     | To remove H <sub>2</sub> S    | To remove H <sub>2</sub> S                   | To remove H <sub>2</sub> S                         |
| <b>Additional Filter</b>  | None                          | Silica filter to improve silicone resistance | Carbon cloth filter to improve silicone resistance |
| <b>Catalogue Listings</b> | PM979-600D-CIT                | PM989-600D-CIT                               | PM999-600D-CIT                                     |

## TECHNICAL SPECIFICATIONS

### MEASUREMENT

|                                |   |
|--------------------------------|---|
| <b>Operating Principle</b>     | Catalytic Oxidation   |
| <b>Range</b>                   | 0 % to 100 % LEL  |
| <b>Inboard Filter Capacity</b> | 1000 ppm hr minimum   |
| <b>Poison Resistance</b>       | Resistant to H <sub>2</sub> S poisoning<br>Superior silicone resistance |
| <b>Response Time*</b>          | <20 seconds to CH <sub>4</sub>  |
| <b>Overload</b>                | 100 % LEL   |
| <b>Output</b>                  | % LEL target gas output<br>Compensated for temperature                  |
| <b>Measurement Interval</b>    | Maximum of 1 sample per second  |
| <b>Linearity*</b>              | Linear up to 5 % vol. CH <sub>4</sub>                                   |
| <b>Measurement Accuracy</b>    | 5 % LEL   |
| <b>Resolution</b>              | 1 % LEL   |
| <b>Lower Deduction Limit</b>   | 4 % LEL   |
| <b>Dead Band</b>               | Configurable  |
| <b>Warm-up Time</b>            | 30 seconds  |
| <b>Serial Communication</b>    | UART with Chip Select   |

### ENVIRONMENTAL

|                                    |  |
|------------------------------------|--|
| <b>Operating Humidity Range</b>    | 0 to 95 % RH (non-condensing)  |
| <b>Operating Pressure Range</b>    | 600 mbar to 1200 mbar  |
| <b>Operating Temperature Range</b> | -20°C to 60°C**<br>** Can be operated from -40°C to -20°C,<br>see characterisation note for details. |
| <b>Flow Rate</b>                   | Typical: 200 ml/min when using<br>recommended gassing hood.<br>(Consult iseries application note)    |

### LIFETIME

|                                 |                                       |
|---------------------------------|---------------------------------------|
| <b>Long-Term Output Drift*</b>  | <3 % signal per month                 |
| <b>Long-Term Baseline Drift</b> | <5 % LEL <sub>methane</sub> per month |
| <b>Expected Operating Life</b>  | 5 years in air                        |

### PHYSICAL CHARACTERISTICS


|                                    |                    |
|------------------------------------|--------------------|
| <b>Weight</b>                      | <6 g               |
| <b>Contact Material</b>            | Gold plated        |
| <b>O-Ring Material</b>             | FKM60 ±5 shore A   |
| <b>Outer Plastic Body Material</b> | PPS Fortron 1140L4 |

\* Specifications are valid at 20°C, 50% RH, and 1013 mBar using City Technology recommended circuitry. Performance characteristics outline the performance of sensors supplied within the first three months. Output signal can drift below the lower limit over time.

## Pinout

| Pin       | Description                                |
|-----------|--|
| <b>+V</b> | Positive power supply                      |
| <b>-V</b> | Ground                                     |
| <b>Rx</b> | Data transmitted from instrument to sensor |
| <b>Tx</b> | Data transmitted from sensor to instrument |
| <b>CS</b> | Chip Select                                |

## Product Dimensions

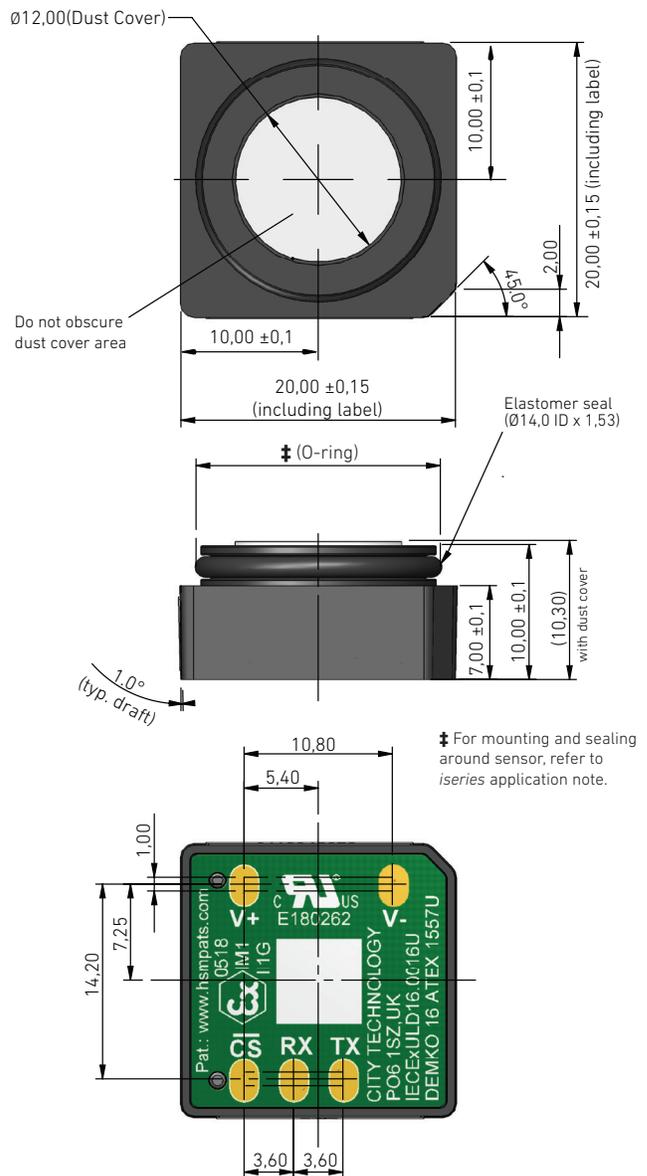

All dimensions in mm

All tolerances ±0,15 mm unless otherwise stated

## Electrical Specifications

|   | Min.  | Max. | Typ. | Unit |
|---|-------|------|------|------|
| <b>Supply voltage (Vdd)</b>                   | 3.1   | 3.3  | 3.2  | Vdc  |
| <b>Voltage on any pin</b>                     | 0     | 3.3  | -    | Vdc  |
| <b>Current: at stand-by mode (sleep mode)</b> | 0.82  | 1.4  | 1.4  | mA   |
| <b>Current: at active mode</b>                | 76    | 90   | 80   | mA   |
| <b>Power consumption at work mode</b>         | 235.6 | 297  | 256  | mW   |
| <b>Start-up time</b>                          | -     | 30   | -    | s    |

For compatibility with the whole iseries range, the supply voltage should be between 3.1 V and 3.3 V.

## iLEL Parameters

| iLEL parameters        |   | Default Values   | Configurable Range  | Customisable: Implemented by City Technology (Non-configurable through the communication protocol) | Configurable: The parameter can be changed through the communication protocol by users | Notes  |
|------------------------|---|--|---|--|--|--|
| OEM Lock               | OEM code (First layer)  | Password is customisable.* ( <b>NoLock</b> will be set by default in case the OEM lock is not required)  | No more than 6 characters (ASCII format)  | ✓  |  | * OEM code will be set by City Technology during sensor manufacturing. Code to be provided by OEM  |
|                        | Partner code (Second layer)                                   | –  | No more than 6 characters (ASCII format)  |  | ✓  | Once this command has been set by user, it won't be possible to change   |
| User Factor            |   | User factor 0: 100<br>User factor 1: 95<br>UF2 to UF9: Customisable<br><br>User factors can be added to include auto-compensation for using different membranes or instruments | 10 allocated slots<br>-----<br><br>2 user factors are already implemented (no additional membrane and with recommended membrane). The remaining 8 can be customised | ✓*   | ✓**  | * User factor 0 and 1 inputted into the sensor during manufacturing. Additional User Factors can be added to the selectable list during the manufacturing process. This user factor has to be provided by the user<br>** Users can select the desired user factor from the selectable list |
| Unit of Measure        |   | % LEL  |   |  | ✓  | The gas concentration can be configured to measure either %LEL or %VOL   |
| Calibration            | Zero (clean air)  | 0 % LEL  |   |  | ✗  | Calibration is performed at two points throughout the operating range of the sensor. The calibration points are defined by the zero and span values. The zero value represent the response of the sensor in clean air  |
|                        | Span (target gas)   | 50 % LEL   |   |  | ✓  | Span is the calibration point that is done in the presence of the target gas. The span concentration can be configured through the communication protocol. The span gas is 50 %LEL, or 2.5 %v/v methane, as per standard EN 50054  |
| Alarms                 | Low   | 10 % LEL   | Limit LOW lower: 3<br>Limit LOW upper: 60   |  | ✓  |  |
|                        | High  | 20 % LEL   | Limit HIGH lower: 3<br>Limit HIGH upper: 60   |  | ✓  |  |
| Predictive calibration | <b>The alarm will be flagged when the countdown reaches 0</b> |  |   |  |  |  |
|                        | Countdown timer (Cal due days)                                | 180 days   |   |  | ✓  | The countdown restarts when the sensor is calibrated. No predictive element for LEL  |
| Target Gas             |   | CH <sub>4</sub>  |   |  | ✓  | The sensor can be configured to measure different target gases. Including CH <sub>4</sub> , C <sub>4</sub> H <sub>10</sub> , H <sub>2</sub> , C <sub>5</sub> H <sub>12</sub> , C <sub>3</sub> H <sub>8</sub>   |
| Calibration Gas        |   | CH <sub>4</sub>  |   |  | ✓  | The sensor can be calibrated with the different gases (CH <sub>4</sub> , C <sub>4</sub> H <sub>10</sub> , H <sub>2</sub> , C <sub>5</sub> H <sub>12</sub> , C <sub>3</sub> H <sub>8</sub> ). It is recommended to calibrate with the target gas  |
| End of Life            | Countdown timer   | 1825 days*   |   |  | ✗  | The countdown timer is set for 1825 days, i.e. 5 years. No predictive element for LEL  |
| Deadband               | Active by default   | ✓  |   |  | ✓  | Deadband is period of dead-state of the sensor where the output is zero. Is normally used to prevent measurement oscillations. This function can be configured to different limits   |
|                        | Incoming  | 1 % LEL  | Whole measurement range   |  | ✓  |  |
|                        | Outgoing  | 3 % LEL  | Incoming ≤ Outgoing   |  | ✓  |  |
| Bump Due Days          |   | 1 day  |   |  | ✓  | A bump test is a brief exposure of the sensor to the target gas. The test has the objective of verifying that the sensor responds and the instrument acts accordingly  |
| Compliance Standard    |   | EN 50054   |   |  |  | The compliance standard measurement can be changed from EN 50054 to EN 60079-20-1  |

## Intrinsic Safety

### Applicable Standards

- UL 913, Intrinsically Safe Apparatus and Associated Apparatus for Use in Class I, II, and III, Division 1, Hazardous (Classified) Locations, Eighth Edition - Revision Date 2019/03/11
- UL 60079-0, Electrical Apparatus for Explosive Atmospheres - Part 0: General Requirements, Seventh Edition - Issue Date 2019/03/26
- UL 60079-1, Electrical Apparatus for Explosive Gas Atmospheres – Part 1: Equipment Protection by Flameproof Enclosures, Seventh Edition – Revision Date 2015/09/18
- UL 60079-11, Electrical Apparatus for Explosive Atmospheres - Part 11: Intrinsic Safety “ia”, Sixth Edition - Revision Date 2018/09/14.
- CAN/CSA-C22.2 No. 157-92, Intrinsically Safe and Non-incendive Equipment for Use in Hazardous Locations - Edition 3 - Revision Date 2003/06/01
- CSA C22.2 NO. 60079-0 Explosive Atmospheres — Part 0: Equipment — General Requirements Edition 4 - Issue Date 2019/02/01
- CSA C22.2 NO. 60079-1:16 Electrical Apparatus for Explosive Gas Atmospheres – Part 1: Flameproof enclosures “d” – Edition 3 – Issue date 2016/05/01
- CSA C22.2 NO. 60079-11:14 Explosive Atmospheres — Part 11: Equipment Protection By Intrinsic Safety “I”- Edition 2 - Issue Date 2014/02/01
- IEC 60079-0 Explosive atmospheres - Part 0: Equipment - General requirements Edition 7 Revision Date 2017
- IEC 60079-1 Electrical Apparatus for Explosive Gas Atmospheres - Part 1: Flame-Proof Enclosures “D” Edition 7 Issue Date 06/2014
- IEC 60079-11 Explosive Atmospheres - Part 11: Equipment Protection by Intrinsic Safety “I” Edition 6 Issue Date 06/2011
- CENELEC EN IEC 60079-0 Explosive Atmospheres - Part 0: Equipment - General Requirements Issue Date 07/22/2018
- CENELEC EN 60079-1 Explosive Atmospheres - Part 1: Equipment Protection by Flameproof Enclosures “D” Issue Date 10/2014
- CENELEC EN 60079-11 Explosive Atmospheres - Part 11: Equipment Protection by Intrinsic Safety “I” Issue Date 02/03/2012
- CENELEC EN 50303 GROUP I, Category M1 Equipment Intended to Remain Functional in Atmospheres Endangered by Firedamp and/or Coal Dust Edition Issue Date 07/2000

## Approvals and Standards

|  |                           |  |
|--|---------------------------|--|
|  | <b>File Number</b>        | E 180262   |
|  | <b>Certificate Number</b> | DEMKO 16 ATEX 1557U<br>IECEX ULD 16.0016U  |
|  | <b>ATEX Marking</b>       | 0518  IM1<br>II1G   |
| <b>Protection<br/>Concept Markings</b> | <b>ATEX Marking</b>       | Ex da ia I Ma<br>Ex da ia IIC Ga   |
|  | <b>UL Marking</b>         | Class 1 Zone 1 AEx da ia IIC Ga  |
|  | <b>Canadian Marking</b>   | Ex da ia I Ma<br>Ex da ia IIC Ga   |
| <b>Electrical data</b>                 | <b>iLEL75X</b>            | Rated voltage: 3.2 V<br>Rated current: 90 mA<br>Rated power: 297 mW  |
|  | <b>iLEL75X</b>            | <b>Intrinsically safe specifications</b><br>U <sub>i</sub> = 5.88 V<br>I <sub>i</sub> = 1.1 A<br>P <sub>i</sub> = 1.2 W<br>L <sub>i</sub> = 0 µH<br>C <sub>i</sub> = 8.38 µF |

### SAFETY NOTE

This sensor is designed to be used in safety-critical applications. To ensure that the sensor and/or instrument in which it is used, are operating properly, it is a requirement that the function of the device is confirmed by exposure to target gas (bump check) before each use of the sensor and/or instrument. Failure to carry out such tests may jeopardize the safety of people and property.

In accordance with the company's policy of continued product improvement City Technology reserves the right to make product changes without notice. The products are always subject to a programme of improvement and testing which may result in some changes in the characteristics quoted. As the products may be used by the client in circumstances beyond the knowledge and control of City Technology, we cannot give any warranty as to the relevance of these particulars to an application. City Technology warrants goods of its manufacture as being free of defective materials and faulty workmanship during the applicable warranty period. City Technology's standard product warranty applies unless agreed to otherwise by City Technology in writing; please refer to your order acknowledgment or consult your local sales office for specific warranty details. If warranted goods are returned to City Technology during the period of coverage, City Technology will repair or replace, at its option, without charge those items that City Technology, in its sole discretion, finds defective. **The foregoing is buyer's sole remedy and is in lieu of all other warranties, expressed or implied, including those of merchantability and fitness for a particular purpose. In no event shall City Technology be liable for consequential, special, or indirect damages.** Though City Technology provides application assistance personally, or through our literature and website, it is buyer's sole responsibility to determine the suitability of the product in the application. Specifications may change without notice. The information we supply is believed to be accurate and reliable as of this writing. However, City Technology assumes no responsibility for its use.